


PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau

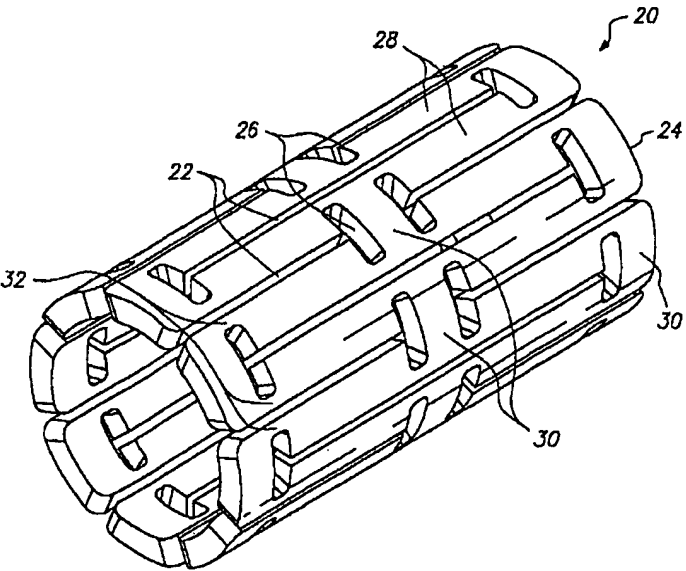

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>6</sup> : <b>A61M 29/00</b>		A1	(11) International Publication Number: <b>WO 99/49928</b>
			(43) International Publication Date: 7 October 1999 (07.10.99)
(21) International Application Number: <b>PCT/US99/06659</b>		(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).	
(22) International Filing Date: 26 March 1999 (26.03.99)			
(30) Priority Data: 60/079,881 30 March 1998 (30.03.98) US 09/183,555 29 October 1998 (29.10.98) US			
(63) Related by Continuation (CON) or Continuation-in-Part (CIP) to Earlier Applications US 60/079,881 (CON) Filed on 30 March 1998 (30.03.98) US 09/183,555 (CON) Filed on 29 October 1998 (29.10.98)		Published With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.	
(71)/(72) Applicant and Inventor: SHANLEY, John, F. [US/US]; 401 Camberly Way, Redwood City, CA 94061 (US).			
(74) Agent: PETERSON, James, W.; Burns, Doane, Swecker & Mathis, L.L.P., P.O. Box 1404, Alexandria, VA 22313-1404 (US).			
(54) Title: EXPANDABLE MEDICAL DEVICE WITH DUCTILE HINGES			
(57) Abstract			
<p>An expandable tissue supporting device (20) of the present invention employs ductile hinges (32) at selected points in the expandable device. When expansion forces are applied to the device as a whole, the ductile hinges concentrate expansion stresses and strains in small well defined areas. The expandable medical device including ductile hinges provides the advantages of low expansion force requirements, relatively thick walls which are radio-opaque, improved crimping properties, high crush strength, reduced elastic recoil after implantation, and control of strain to a desired level. The expandable tissue supporting device includes a plurality of elongated beams arranged in a cylindrical device and connected together by a plurality of ductile hinges. Although many ductile hinge configurations are possible, the ductile hinges preferably have a substantially constant hinge cross-sectional area which is smaller than a beam cross-sectional area such that as the device is expanded from a first diameter to a second diameter, the ductile hinges experience plastic deformation while the beams are not plastically deformed.</p>			
			

BEST AVAILABLE COPY

*FOR THE PURPOSES OF INFORMATION ONLY*

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakhstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

**EXPANDABLE MEDICAL DEVICE WITH DUCTILE HINGES**  
**BACKGROUND OF THE INVENTION**

**1. Field of the Invention**

The present invention relates to tissue-supporting medical devices, and more particularly to expandable, non-removable devices that are implanted within a bodily lumen of a living animal or human to support the organ and maintain patency.

**2. Summary of the Related Art**

In the past, permanent or biodegradable devices have been developed for implantation within a body passageway to maintain patency of the passageway. These devices are typically introduced percutaneously, and transported transluminally until positioned at a desired location. These devices are then expanded either mechanically, such as by the expansion of a mandrel or balloon positioned inside the device, or expand themselves by releasing stored energy upon actuation within the body. Once expanded within the lumen, these devices, called stents, become encapsulated within the body tissue and remain a permanent implant.

Known stent designs include monofilament wire coil stents (U.S. Pat. No. 4,969,458); welded metal cages (U.S. Pat. Nos. 4,733,665 and 4,776,337); and, most prominently, thin-walled metal cylinders with axial slots formed around the circumference (U.S. Pat. Nos. 4,733,665, 4,739,762, and 4,776,337). Known construction materials for use in stents include polymers, organic fabrics and biocompatible metals, such as, stainless steel, gold, silver, tantalum, titanium, and shape memory alloys such as Nitinol.

-2-

U.S. Pat. Nos. 4,733,665, 4,739,762, and 4,776,337 disclose expandable and deformable interluminal vascular grafts in the form of thin-walled tubular members with axial slots allowing the members to be expanded radially outwardly into contact with a body passageway. After insertion, the tubular members are mechanically expanded beyond their elastic limit and thus permanently fixed within the body. The force required to expand these tubular stents is proportional to the thickness of the wall material in a radial direction. To keep expansion forces within acceptable levels for use within the body (e.g., 5 - 10 atm), these designs must use very thin-walled materials (e.g., stainless steel tubing with 0.0025 inch thick walls). However, materials this thin are not visible on conventional fluoroscopic and x-ray equipment and it is therefore difficult to place the stents accurately or to find and retrieve stents that subsequently become dislodged and lost in the circulatory system.

Further, many of these thin-walled tubular stent designs employ networks of long, slender struts whose width in a circumferential direction is two or more times greater than their thickness in a radial direction. When expanded, these struts are frequently unstable, that is, they display a tendency to buckle, with individual struts twisting out of plane. Excessive protrusion of these twisted struts into the bloodstream has been observed to increase turbulence, and thus encourage thrombosis. Additional procedures have often been required to attempt to correct this problem of buckled struts. For example, after initial stent implantation is determined to have caused buckling of struts, a second, high-pressure balloon (e.g., 12 to 18 atm) would be used to attempt to drive the twisted struts further into the lumen wall. These secondary procedures can be dangerous to the patient due to the risk of collateral damage to the lumen wall.

Many of the known stents display a large elastic recovery, known in the field as "recoil," after expansion inside a lumen. Large recoil necessitates over-expansion of the stent during implantation to achieve the desired final diameter. Over-expansion is potentially destructive to the lumen tissue. Known

-3-

stents of the type described above experience recoil of up to about 6 to 12% from maximum expansion.

Large recoil also makes it very difficult to securely crimp most known stents onto delivery catheter balloons. As a result, slippage of stents on balloons during interluminal transportation, final positioning, and implantation has been an ongoing problem. Many ancillary stent securing devices and techniques have been advanced to attempt to compensate for this basic design problem. Some of the stent securing devices include collars and sleeves used to secure the stent onto the balloon.

Another problem with known stent designs is non-uniformity in the geometry of the expanded stent. Non-uniform expansion can lead to non-uniform coverage of the lumen wall creating gaps in coverage and inadequate lumen support. Further, over expansion in some regions or cells of the stent can lead to excessive material strain and even failure of stent features. This problem is potentially worse in low expansion force stents having smaller feature widths and thicknesses in which manufacturing variations become proportionately more significant. In addition, a typical delivery catheter for use in expanding a stent includes a balloon folded into a compact shape for catheter insertion. The balloon is expanded by fluid pressure to unfold the balloon and deploy the stent. This process of unfolding the balloon causes uneven stresses to be applied to the stent during expansion of the balloon due to the folds causing the problem non-uniform stent expansion.

U.S. Pat. No. 5,545,210 discloses a thin-walled tubular stent geometrically similar to those discussed above, but constructed of a nickel-titanium shape memory alloy ("Nitinol"). This design permits the use of cylinders with thicker walls by making use of the lower yield stress and lower elastic modulus of martensitic phase Nitinol alloys. The expansion force required to expand a Nitinol stent is less than that of comparable thickness stainless steel stents of a conventional design. However, the "recoil" problem after expansion is

-4-

significantly greater with Nitinol than with other materials. For example, recoil of a typical design Nitinol stent is about 9%. Nitinol is also more expensive, and more difficult to fabricate and machine than other stent materials, such as stainless steel.

All of the above stents share a critical design property: in each design, the features that undergo permanent deformation during stent expansion are prismatic, i.e., the cross sections of these features remain constant or change very gradually along their entire active length. To a first approximation, such features deform under transverse stress as simple beams with fixed or guided ends: essentially, the features act as a leaf springs. These leaf spring like structures are ideally suited to providing large amounts of elastic deformation before permanent deformation commences. This is exactly the opposite of ideal stent behavior. Further, the force required to deflect prismatic stent struts in the circumferential direction during stent expansion is proportional to the square of the width of the strut in the circumferential direction. Expansion forces thus increase rapidly with strut width in the above stent designs. Typical expansion pressures required to expand known stents are between about 5 and 10 atmospheres. These forces can cause substantial damage to tissue if misapplied.

FIG. 1 shows a typical prior art "expanding cage" stent design. The stent 10 includes a series of axial slots 12 formed in a cylindrical tube 14. Each axial row of slots 12 is displaced axially from the adjacent row by approximately half the slot length providing a staggered slot arrangement. The material between the slots 12 forms a network of axial struts 16 joined by short circumferential links 18. The cross section of each strut 16 remains constant or varies gradually along the entire length of the strut and thus the rectangular moment of inertia and the elastic and plastic section moduli of the cross section also remain constant or vary gradually along the length of the strut. Such a strut 16 is commonly referred to as a prismatic beam. Struts 16 in this type of design are typically 0.005 to 0.006 inches (0.127 - 0.1524 mm) wide in the circumferential direction. Strut

-5-

thicknesses in the radial direction are typically about 0.0025 inches (0.0635 mm) or less to keep expansion forces within acceptable levels. However, most stent materials must be approximately 0.005 inches (0.127 mm) thick for good visibility on conventional fluoroscopic equipment. This high ratio of strut width to thickness, combined with the relatively high strut length and the initial curvature of the stent tubing combine to cause the instability and bucking often seen in this type of stent design. When expanded, the stent structure of FIG. 1 assumes the roughly diamond pattern commonly seen in expanded sheet metal.

Another stent described in PCT publication number WO 96/29028 uses struts with relatively weak portions of locally-reduced cross sections which on expansion of the stent act to concentrate deformation at these areas. However, as discussed above non-uniform expansion is even more of a problem when smaller feature widths and thicknesses are involved because manufacturing variations become proportionately more significant. The locally-reduced cross section portions described in this document are formed by pairs of circular holes. The shape of the locally-reduced cross section portions undesirably concentrates the plastic strain at the narrowest portion. This concentration of plastic strain without any provision for controlling the level of plastic strain makes the stent highly vulnerable to failure.

In view of the drawbacks of the prior art stents, it would be advantageous to be able to expand a stent with an expansion force at a low level independent of choice of stent materials, material thickness, or strut dimensions.

It would further be advantageous to have a tissue-supporting device that permits a choice of material thickness that could be viewed easily on conventional fluoroscopic equipment for any material.

It would also be advantageous to have a tissue-supporting device that is inherently stable during expansion, thus eliminating buckling and twisting of structural features during stent deployment.

-6-

It would also be desirable to control strain to a desired level which takes advantage of work hardening without approaching a level of plastic strain at which failure may occur.

In addition, it would be advantageous to have a tissue-supporting device with minimal elastic recovery, or "recoil" of the device after expansion.

It would be advantageous to have a tissue supporting device that can be securely crimped to the delivery catheter without requiring special tools, techniques, or ancillary clamping features.

It would further be advantageous to have a tissue-supporting device that has improved resistance to compressive forces (improved crush strength) after expansion.

It would also be advantageous to have a tissue-supporting device that achieves all the above improvements with minimal foreshortening of the overall stent length during expansion.

#### **SUMMARY OF THE INVENTION**

The present invention addresses several important problems in expandable medical device design including: high expansion force requirements; lack of radio-opacity in thin-walled stents; buckling and twisting of stent features during expansion; poor crimping properties; and excessive elastic recovery ("recoil") after implantation. The invention also provides benefits of improved resistance to compressive forces after expansion, control of the level of plastic strain, and low axial shortening during expansion. Some embodiments of the invention also provide improved uniformity of expansion by limiting a maximum geometric deflection between struts. The invention may also incorporate sites for the inclusion of beneficial agent delivery.

The invention involves the incorporation of stress/strain concentration features or "ductile hinges" at selected points in the body of an expandable cylindrical medical device. When expansion forces are applied to the device as a



-7-

whole, these ductile hinges concentrate expansion stresses and strains in small, well-defined areas while limiting strut deflection and plastic strain to specified levels.

In accordance with one aspect of the present invention, an expandable medical device includes a plurality of elongated beams having a substantially constant beam cross sectional area along a beam length. The plurality of elongated beams are joined together to form a substantially cylindrical device which is expandable from a cylinder having a first diameter to a cylinder having a second diameter. A plurality of ductile hinges connect the plurality of beams together in the substantially cylindrical device. The ductile hinges have a substantially constant hinge cross sectional area along a substantial portion of a hinge length. The hinge cross sectional area is smaller than the beam cross sectional area such that as the device is expanded from the first diameter to the second diameter the ductile hinges experience plastic deformation while the beams are not plastically deformed.

In accordance with a further aspect of the invention, an expandable medical device includes a cylindrical tube, and a plurality of axial slots formed in the cylindrical tube in a staggered arrangement to define a network of elongated struts, wherein each of the elongated struts are axially displaced from adjacent struts. A plurality of ductile hinges are formed between the elongated struts. The ductile hinges allow the cylindrical tube to be expanded or compressed from a first diameter to a second diameter by deformation of the ductile hinges. The ductile hinges are asymmetrically configured to reach a predetermined strain level upon a first percentage expansion and to reach the predetermined strain level upon a second percentage of compression, wherein the first percentage is larger than the second percentage.

In accordance with another aspect of the present invention, an expandable medical device includes a plurality of elongated beams having a substantially constant beam cross sectional area along a beam length. A plurality of ductile

-8-

hinges connect the plurality of beams together in a substantially cylindrical device which is expandable or compressible from a first diameter to a second diameter by plastic deformation of the ductile hinges. A plurality of deflection limiting members are positioned at a plurality of the ductile hinges which limit the deflection at the ductile hinges.

#### **BRIEF DESCRIPTION OF THE DRAWINGS**

The invention will now be described in greater detail with reference to the preferred embodiments illustrated in the accompanying drawings, in which like elements bear like reference numerals, and wherein:

FIG. 1 is an isometric view of a prior art tissue-supporting device;

FIG. 2 is an isometric view of a tissue-supporting device in accordance with one embodiment of the invention;

FIGS. 3a-d are perspective views of ductile hinges according to several variations of the invention;

FIG. 3e is a side view of another embodiment of a ductile hinge;

FIGS. 4a and 4b are an isometric view and an enlarged side view of a tissue-supporting device in accordance with an alternative embodiment of the invention;

FIGS. 5a-c are perspective, side, and cross-sectional views of an idealized ductile hinge for purposes of analysis;

FIG. 5d is a stress/strain curve for the idealized ductile hinge;

FIGS. 6 is a perspective view of a simple beam for purposes of calculation;

FIG. 7 is a moment verses curvature graph for a rectangular beam;

FIG. 8 is an enlarged side view of a bent ductile hinge;

FIGS. 9a and 9b are enlarged side views of ductile hinges in initial and expanded positions with shortened struts to illustrate axial contraction relationships; and

-9-

FIG. 10 is a side view of a portion of an alternative embodiment of a tissue supporting device having a high-crush-strength and low-recoil.

#### **DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS**

FIG. 2 shows one embodiment of an expandable tissue supporting device 20 in accordance with the present invention. The tissue supporting device 20 includes a series of axial slots 22 formed in a cylindrical tube 24. Each axial slot 22 is displaced axially from the slots in adjacent rows of slots by approximately half the slot length resulting in a staggered slot arrangement. The offset between adjacent rows of slots results in alternate rows of slots which extend to the ends of the cylindrical tube 24. At each interior end of each of the axial slots 22 a circumferential slot 26 is formed. The material between the slots 22 forms a network of axial struts 28 extending substantially parallel to an axis of the tube 24. The axial struts 28 are joined by short circumferential links 30. The circumferential links 30 are positioned at both the interior of the cylindrical tube and at the ends of the cylindrical tube. The cross section (and rectangular moment of inertia) of each of the struts 28 is not constant along the length of the strut. Rather, the strut cross section changes abruptly at both ends of each strut 28 at the location of the circumferential slots 26. The struts 28 are thus not prismatic. Each individual strut 28 is linked to the rest of the structure through a pair of reduced sections 32, one at each end, which act as stress/strain concentration features. The reduced sections 32 of the struts function as hinges in the cylindrical structure. Since the stress/strain concentration features 32 are designed to operate into the plastic deformation range of generally ductile materials, they are referred to as ductile hinges. Such features are also commonly referred to as "Notch Hinges" or "Notch Springs" in ultra-precision mechanism design, where they are used exclusively in the elastic range.

With reference to the drawings and the discussion, the *width* of any feature is defined as its dimension in the circumferential direction of the cylinder. The

-10-

*length* of any feature is defined as its dimension in the axial direction of the cylinder. The *thickness* of any feature is defined as the wall thickness of the cylinder.

The presence of the ductile hinges 32 allows all of the remaining features in the tissue supporting device to be increased in width or the circumferentially oriented component of their respective rectangular moments of inertia - thus greatly increasing the strength and rigidity of these features. The net result is that elastic, and then plastic deformation commence and propagate in the ductile hinges 32 before other structural elements of the device undergo any significant elastic deformation. The force required to expand the tissue supporting device 20 becomes a function of the geometry of the ductile hinges 32, rather than the device structure as a whole, and arbitrarily small expansion forces can be specified by changing hinge geometry for virtually any material wall thickness. In particular, wall thicknesses great enough to be visible on a fluoroscope can be chosen for any material of interest.

In order to get minimum recoil, the ductile hinges 32 should be designed to operate well into the plastic range of the material, and relatively high local strain-curvatures are developed. When these conditions apply, elastic curvature is a very small fraction of plastic or total curvature, and thus when expansion forces are relaxed, the percent change in hinge curvature is very small. When incorporated into a strut network designed to take maximum advantage of this effect, the elastic springback, or "recoil," of the overall stent structure is minimized.

In the embodiment of FIG. 2, it is desirable to increase the width of the individual struts 28 between the ductile hinges 32 to the maximum width that is geometrically possible for a given diameter and a given number of struts arrayed around that diameter. The only geometric limitation on strut width is the minimum practical width of the slots 22 which is about 0.002 inches (0.0508 mm) for laser machining. Lateral stiffness of the struts 28 increases as the cube of strut

-11-

width, so that relatively small increases in strut width significantly increase strut stiffness. The net result of inserting ductile hinges 32 and increasing strut width is that the struts 28 no longer act as flexible leaf springs, but act as essentially rigid beams between the ductile hinges. All radial expansion or compression of the cylindrical tissue supporting device 20 is accommodated by mechanical strain in the hinge features 32, and yield in the hinge commences at very small overall radial expansion or compression.

Yield in ductile hinges at very low gross radial deflections also provides the superior crimping properties displayed by the ductile hinge-based designs. When a tissue supporting device is crimped onto a folded catheter balloon, very little radial compression of the device is possible since the initial fit between balloon and device is already snug. Most stents simply rebound elastically after such compression, resulting in very low clamping forces and the attendant tendency for the stent to slip on the balloon. Ductile hinges, however, sustain significant plastic deformation even at the low deflections occurring during crimping onto the balloon, and therefore a device employing ductile hinges displays much higher clamping forces. The ductile hinge designs according to the present invention may be securely crimped onto a balloon of a delivery catheter by hand or by machine without the need for auxiliary retaining devices commonly used to hold known stents in place.

The geometric details of the stress/strain concentration features or ductile hinges 32 can be varied greatly to tailor the exact mechanical expansion properties to those required in a specific application. The most obvious and straightforward ductile hinges are formed by slots or notches with rounded roots, as in FIGS. 3a and 3c. Since the laser beams often used to fabricate these features are themselves round, slots or notches with circular roots are also among the easiest to fabricate.

FIG. 3a shows a ductile hinge 36 formed by a pair of opposed circular grooves 38, 40. According to this embodiment the circumferential slot 26 has semicircular ends 38 having a radius of curvature  $r$ . Outer semicircular grooves

-12-

40 opposed the semicircular ends 38 and also have a radius of curvature  $r$ . FIG. 3c shows another ductile hinge 54 formed by a parabolic groove 56.

Generally, the ductile hinges 36 of the embodiment of FIG. 3a formed between pairs of concave curves 38, 40 have a minimum width along a line connecting their respective centers of curvature. When the struts connected by the ductile hinge are moved apart or together, plastic deformation is highly concentrated in a region immediately adjacent to the plane that bisects the hinge at this narrow point.

For smaller deflection, this very high strain concentration at the bisecting plane is acceptable, and in some cases, useful. For stent crimping purposed, for example, it is desirable to generate relatively large plastic deformations at very small deflection angles.

As a practical matter, however, strut deflection angles for device *expansion* are often in the 25° to 45° range. At these angles, strain at the root or bisecting plane of concave ductile hinge features can easily exceed the 50 to 60% elongation-to-failure of 316L stainless steel, one of the most ductile stent materials. Deflection limiting features which will be described further below limit the *geometric* deflection of struts, but these features do not in themselves affect the propagation pattern of plastic deformation in a given ductile hinge design. For concave ductile hinges at large bend angles, very high strain concentrations remain. Scanning electron micrographs have confirmed this analysis.

In many engineering applications, it is desirable to limit the amount of strain, or "cold-work," in a material to a specified level in order to optimize material properties and to assure safe operation. For example, in medical applications it is desirable to limit the amount of cold-work in 316L stainless steel to about 30%. At this level, the strength of the material is increased, while the material strain is still well below the failure range. Ideally, therefore, a safe and effective ductile hinge should not simply limit gross deflection, but reliably limit *material strain* to a specified level.

-13-

FIG. 3b shows a simple ductile hinge design that allows material strain to be limited to some specified level. The ductile hinge of FIG. 3b is formed by a rectangular circumferential groove 46 with filleted corners 48 on one side of a strut, the opposite side 50 of the strut remaining straight. The ductile hinges 44 are substantially rectangular sections between the ends of the groove 46 and the side walls 50.

One of the key concepts in FIG. 3b is that the ductile hinge 44 has a constant or substantially constant width along at least a portion of its total length. In this configuration, there is no local minimum width along the ductile hinge axis, as there is with pairs of concave roots. There is therefore no point concentration of stresses and strains along the length of the ductile hinge beam during stent expansion. In particular, maximum tensile and compressive strains will be distributed evenly along the upper and lower surfaces of the hinge 44 during stent expansion. With the gross bend angle limited by mechanical stops, which are described below in detail, the maximum *material strain* (at the hinge surfaces) can therefore be reliably limited by adjusting the initial length of the ductile hinge over which the total elongation is distributed.

FIG. 3d shows a ductile hinge 60 in a cylindrical wire 62 for incorporating into a wire-form tissue-supporting device. The ductile hinge 60 is formed by a reduced diameter portion of the wire 62. Again, it is important that the ductile hinge have a substantially constant width over a portion of its length in order to provide strain control. Preferably, the ductile hinge is prismatic over a portion of its length. Maximum material strain can be varied by adjusting the hinge length. The ductile hinges of the present invention have a constant or substantially constant width over at least 1/3 of the ductile hinge length, and preferably over at least 1/2 of the ductile hinge length.

FIG. 3e shows an asymmetric ductile hinge 63 that produces different strain versus deflection-angle functions in expansion and compression. Each of the ductile hinges 64 is formed between a convex surface 68 and a concave surface 69.

-14-

The ductile hinge 64 according to a preferred embodiment essentially takes the form of a small, prismatic curved beam having a substantially constant cross section. However, a thickness of the curved ductile hinge 64 may vary somewhat as long as the ductile hinge width remains constant along a portion of the hinge length. The width of the curved beam is measure along the radius of curvature of the beam. This small curved beam is oriented such that the smaller *concave* surface 69 is placed in tension in the device *crimping* direction, while the larger *convex* surface 68 of the ductile hinges is placed in tension in the device *expansion* direction. Again, there is no local minimum width of the ductile hinge 64 along the (curved) ductile hinge axis, and no concentration of material strain. During device expansion tensile strain will be distributed along the convex surface 68 of the hinge 64 and maximum expansion will be limited by the angle of the walls of the concave notch 69 which provide a geometric deflection limiting feature. Maximum tensile strain can therefore be reliably limited by adjusting the initial length of the convex arc shaped ductile hinge 64 over which the total elongation is distributed.

The ductile hinges illustrated in FIGS. 3a-e are examples of different structures that will function as a stress/strain concentrator. Many other stress/strain concentrator configurations may also be used as the ductile hinges in the present invention. The ductile hinges according to the present invention generally include an abrupt change in width of a strut that functions to concentrate stresses and strains in the narrower section of the strut. These ductile hinges also generally include features to limit mechanical deflection of attached struts and features to control material strain during large strut deflections. Although the ductile hinges have been illustrated in FIG. 2 as positioned at the ends of each of the axial slots 22, they may also be positioned at other locations in other designs without departing from the present invention.

An alternative embodiment of a tissue supporting device 80 is illustrated in FIG. 4a and in the enlarged side view of FIG. 4b. The tissue supporting device 80



-15-

includes a plurality of cylindrical tubes 82 connected by S-shaped bridging elements 84. The bridging elements 84 allow the tissue supporting device to bend axially when passing through the tortuous path of the vasculature to the deployment site and allow the device to bend when necessary to match the curvature of a lumen to be supported. The S-shaped bridging elements 84 provide improved axial flexibility over prior art devices due to the thickness of the elements in the radial direction which allows the width of the elements to be relatively small without sacrificing radial strength. For example, the width of the bridging elements 84 may be about 0.0012 - 0.0013 inches (0.0305 - 0.0330 mm). Each of the cylindrical tubes 82 has a plurality of axial slots 86 extending from an end surface of the cylindrical tube toward an opposite end surface. A plurality of axial struts 88 having ductile hinges 90 are formed between the axial slots 86. The ductile hinges 90 are formed by circumferential slots 92 formed at the interior ends of the axial slots 86 and opposed notches 94.

The notches 94 each have two opposed angled walls 96 which function as a stop to limit geometric deflection of the ductile hinge, and thus limit maximum device expansion. As the cylindrical tubes 82 are expanded and bending occurs at the ductile hinges 90, the angled side walls 96 of the notches 94 move toward each other. Once the opposite side walls 96 of a notch come into contact with each other, they resist further expansion of the particular ductile hinge causing further expansion to occur at other sections of the tissue supporting device. This geometric deflection limiting feature is particularly useful where uneven expansion is caused by either variations in the tissue supporting device 80 due to manufacturing tolerances or uneven balloon expansion.

The tissue supporting device 20, 80 according to the present invention may be formed of any ductile material, such as steel, gold, silver, tantalum, titanium, Nitinol, other shape memory alloys, other metals, or even some plastics. One preferred method for making the tissue supporting device 20, 80 involves forming a cylindrical tube and then laser cutting the slots 22, 26, 86, 92 and notches 94

-16-

into the tube. Alternatively, the tissue supporting device may be formed by electromachining, chemical etching followed by rolling and welding, or any other known method.

The design and analysis of stress/strain concentration for ductile hinges, and stress/strain concentration features in general, is complex. For example, the stress concentration factor for the simplified ductile hinge geometry of FIG. 3a can be calculated and is given by the following expression where D is the width of the struts 28, h is the height of the circular grooves 38, 40, and r is the radius of curvature of the grooves. For purposes of this example the ratio of h/r is taken to be 4. However, other ratios of h/r can also be implemented successfully.

$$K = 4.935 - 7.586 \left( \frac{2h}{D} \right) + 0.515 \left( \frac{2h}{D} \right)^2 + 0.432 \left( \frac{2h}{D} \right)^3$$

The stress concentration factors are generally useful only in the linear elastic range. Stress concentration patterns for a number of other geometries can be determined through photoelastic measurements and other experimental methods. Stent designs based on the use of stress/strain concentration features, or ductile hinges, generally involve more complex hinge geometries and operate in the non-linear elastic and plastic deformation regimes.

The general nature of the relationship among applied forces, material properties, and ductile hinge geometry can be more easily understood through analysis of an idealized hinge 66 as shown in FIGS. 5a-5c. The hinge 66 is a simple beam of rectangular cross section having a width h, length L and thickness b. The idealized hinge 66 has elastic-ideally-plastic material properties which are characterized by the ideal stress/strain curve of FIG. 5d. It can be shown that the

-17-

"plastic" or "ultimate bending moment" for such a beam is given by the expression:

$$M_p \equiv M_{ult} = \delta_{yp} \frac{bh^2}{4}$$

Where b corresponds to the cylindrical tube wall thickness, h is the circumferential width of the ductile hinge, and  $\delta_{yp}$  is the yield stress of the hinge material. Assuming only that expansion pressure is proportional to the plastic moment, it can be seen that the required expansion pressure to expand the tissue supporting device increases *linearly* with wall thickness b and as the *square* of ductile hinge width h. It is thus possible to compensate for relatively large changes in wall thickness b with relatively small changes in hinge width h. While the above idealized case is only approximate, empirical measurements of expansion forces for different hinge widths in several different ductile hinge geometries have confirmed the general form of this relationship. Accordingly, for different ductile hinge geometries it is possible to increase the thickness of the tissue supporting device to achieve radiopacity while compensating for the increased thickness with a much smaller decrease in hinge width.

Ideally, the stent wall thickness b should be as thin as possible while still providing good visibility on a fluoroscope. For most stent materials, including stainless steel, this would suggest a thickness of about 0.005 - 0.007 inches (0.127 - 0.178 mm) or greater. The inclusion of ductile hinges in a stent design can lower expansion forces/pressures to very low levels for any material thickness of interest. Thus ductile hinges allow the construction of optimal wall thickness tissue supporting devices at expansion force levels significantly lower than current non-visible designs.

The expansion forces required to expand the tissue supporting device 20 according to the present invention from an initial condition illustrated in FIG. 2 to an expanded condition is between 1 and 5 atmospheres, preferably between 2 and

-18-

3 atmospheres. The expansion may be performed in a known manner, such as by inflation of a balloon or by a mandrel. The tissue supporting device 20 in the expanded condition has a diameter which is preferably up to three times the diameter of the device in the initial unexpanded condition.

Many tissue supporting devices fashioned from cylindrical tubes comprise networks of long, narrow, prismatic beams of essentially rectangular cross section as shown in FIG. 6. These beams which make up the known tissue supporting devices may be straight or curved, depending on the particular design. Known expandable tissue supporting devices have a typical wall thickness  $b$  of 0.0025 inches (0.0635 mm), and a typical strut width  $h$  of 0.005 to 0.006 inches (0.127 - 0.1524 mm). The ratio of  $b:h$  for most known designs is 1:2 or lower. As  $b$  decreases and as the beam length  $L$  increases, the beam is increasingly likely to respond to an applied bending moment  $M$  by buckling, and many designs of the prior art have displayed this behavior. This can be seen in the following expression for the "critical buckling moment" for the beam of FIG. 6.

$$M_{crit} = \frac{\pi b^3 h \sqrt{EG(1 - 0.63 \ b/h)}}{6L}$$

Where:  $E$  = Modulus of Elasticity

$G$  = Shear Modulus

By contrast, in a ductile hinge based design according to the present invention, only the hinge itself deforms during expansion. The typical ductile hinge 32 is not a long narrow beam as are the struts in the known stents. Wall thickness of the present invention may be increased to 0.005 inches (0.127 mm) or greater, while hinge width is typically 0.002 - 0.003 inches (0.0508 - 0.0762 mm), preferably 0.0025 inches (0.0635 mm) or less. Typical hinge length, at 0.002 to 0.005 inches (0.0508 - 0.0127 mm), is more than an order of magnitude less than typical strut length. Thus, the ratio of  $b:h$  in a typical ductile hinge 32 is 2:1 or greater. This is an inherently stable ratio, meaning that the plastic moment for

-19-

such a ductile hinge beam is much lower than the critical buckling moment  $M_{crit}$ , and the ductile hinge beam deforms through normal strain-curvature. Ductile hinges 32 are thus not vulnerable to buckling when subjected to bending moments during expansion of the tissue supporting device 20.

To provide optimal recoil and crush-strength properties, it is desirable to design the ductile hinges so that relatively large strains, and thus large curvatures, are imparted to the hinge during expansion of the tissue supporting device. Curvature is defined as the reciprocal of the radius of curvature of the neutral axis of a beam in pure bending. A larger curvature during expansion results in the elastic curvature of the hinge being a small fraction of the total hinge curvature. Thus, the gross elastic recoil of the tissue supporting device is a small fraction of the total change in circumference. It is generally possible to do this because common stent materials, such as 316L Stainless Steel have very large elongations-to-failure (i.e., they are very ductile).

It is not practical to derive exact expressions for residual curvatures for complex hinge geometries and real materials (i.e., materials with non-idealized stress/strain curves). The general nature of residual curvatures and recoil of a ductile hinge may be understood by examining the moment-curvature relationship for the elastic-ideally-plastic rectangular hinge 66 shown in FIGS. 5a-c. It may be shown that the relationship between the applied moment and the resulting beam curvature is:

$$M = M_p \left[ 1 - \frac{1}{3} \left( \frac{y}{h/2} \right)^2 \right] = \frac{3}{2} M_{yp} \left[ 1 - \frac{1}{3} \left( \frac{\kappa}{\kappa_{yp}} \right)^2 \right]$$

This function is plotted in FIG. 7. It may be seen in this plot that the applied moment  $M$  asymptotically approaches a limiting value  $M_p$ , called the plastic or ultimate moment. Beyond  $11/12 M_p$  large plastic deformations occur with little additional increase in applied moment. When the applied moment is removed, the beam rebounds elastically along a line such as a-b. Thus, the elastic portion of the

-20-

total curvature approaches a limit of 3/2 the curvature at the yield point. These relations may be expressed as follows:

$$M_p = \frac{3}{2} M_{yp} \Rightarrow \kappa_{rebound} = \frac{3}{2} \kappa_{yp}$$

Imparting additional curvature in the plastic zone cannot further increase the elastic curvature, but *will* decrease the ratio of elastic to plastic curvature. Thus, additional curvature or larger expansion of the tissue supporting device will reduce the percentage recoil of the overall stent structure.

As shown in FIG. 8, when a rigid strut 28 is linked to the ductile hinge 66 described above, the strut 28 forms an angle  $\theta$  with the horizontal that is a function of hinge curvature. A change in hinge curvature results in a corresponding change in this angle  $\theta$ . The angular elastic rebound of the hinge is the change in angle  $\Delta \theta$  that results from the rebound in elastic curvature described above, and thus angular rebound also approaches a limiting value as plastic deformation proceeds. The following expression gives the limiting value of angular elastic rebound for the idealized hinge of FIG. 8.

$$\theta_{rebound} = 3 \epsilon_{yp} \frac{L}{h}$$

Where strain at the yield point is an independent material property (yield stress divided by elastic modulus); L is the length of the ductile hinge; and h is the width of the hinge. For non-idealized ductile hinges made of real materials, the constant 3 in the above expression is replaced by a slowly rising function of total strain, but the effect of geometry would remain the same. Specifically, the elastic rebound angle of a ductile hinge decreases as the hinge width h increases, and increases as the hinge length L increases. To minimize recoil, therefore, hinge width h should be increased and length L should be decreased.

-21-

Ductile hinge width  $h$  will generally be determined by expansion force criteria, so it is important to reduce hinge length to a practical minimum in order to minimize elastic rebound. Empirical data on recoil for ductile hinges of different lengths show significantly lower recoil for shorter hinge lengths, in good agreement with the above analysis.

The ductile hinges 32 of the tissue supporting device 20 provide a second important advantage in minimizing device recoil. The embodiment of FIG. 2 shows a network of struts joined together through ductile hinges to form a cylinder. In this design, the struts 28 are initially parallel to an axis of the device. As the device is expanded, curvature is imparted to the hinges 32, and the struts 28 assume an angle  $\theta$  with respect to their original orientation, as shown in FIG. 8. The total circumferential expansion of the tissue supporting device structure is a function of hinge curvature (strut angle) and strut length. Moreover, the incremental contribution to stent expansion (or recoil) for an individual strut depends on the instantaneous strut angle. Specifically, for an incremental change in strut angle  $\Delta\theta$ , the incremental change in circumference  $\Delta C$  will depend on the strut length  $R$  and the cosine of the strut angle  $\theta$ .

$$\Delta C = R \Delta\theta \cos\theta$$

Since elastic rebound of hinge curvature is nearly constant at any gross curvature, the net contribution to circumferential recoil  $\Delta C$  is lower at higher strut angles  $\theta$ . The final device circumference is usually specified as some fixed value, so decreasing overall strut length can increase the final strut angle  $\theta$ . Total stent recoil can thus be minimized with ductile hinges by using shorter struts and higher hinge curvatures when expanded.

Empirical measurements have shown that tissue supporting device designs based on ductile hinges, such as the embodiment of FIG. 2, display superior resistance to compressive forces once expanded despite their very low expansion force. This asymmetry between compressive and expansion forces may be due to

-22-

a combination of factors including the geometry of the ductile hinge, the increased wall thickness, and increased work hardening due to higher strain levels.

According to one example of the tissue supporting device of the invention, the device can be expanded by application of an internal pressure of about 2 atmospheres or less, and once expanded to a diameter between 2 and 3 times the initial diameter can withstand a compressive force of about 16 to 20 gm/mm or greater. Examples of typical compression force values for prior art devices are 3.8 to 4.0 gm/mm.

While both recoil and crush strength properties of tissue supporting devices can be improved by use of ductile hinges with large curvatures in the expanded configuration, care must be taken not to exceed an acceptable maximum strain level for the material being used. For the ductile hinge 44 of FIG. 3b, for example, it may be shown that the maximum material strain for a given bend angle is given by the expression:

$$\epsilon_{\max} = \frac{h}{L} \frac{\theta}{2}$$

Where  $\epsilon_{\max}$  is maximum strain, h is ductile hinge width, L is ductile hinge length and  $\theta$  is bend angle in radians. When strain, hinge width and bend angle are determined through other criteria, this expression can be evaluated to determine the correct ductile hinge length L.

For example, suppose the ductile hinge 44 of FIG. 3b was to be fabricated of 316L stainless steel with a maximum strain of 30%; ductile hinge width h is set at 0.0025 inch (0.0635 mm) by expansion force criteria; and the bend angle  $\theta$  is mechanically limited to 0.5 radians ( $\approx 30^\circ$ ) at full stent expansion. Solving the above expression for L gives the required ductile hinge length of at least about 0.0033 inches (0.0838 mm).



Similar expressions may be developed to determine required lengths for more complicated ductile hinge geometries, such as shown in FIG. 3e. Typical values for the prismatic portions of these curved ductile hinges range from about 0.002 to about 0.0035 inches (0.051 - 0.089 mm) in hinge width and about 0.002 to about 0.006 inches (0.051 - 0.152 mm) in hinge length. The tissue supporting device design of FIGS. 4a and 4b include a stop which limits the maximum geometric deflection at the ductile hinges by the design of the angled walls 96 of the notches 94.

In many designs of the prior art, circumferential expansion was accompanied by a significant contraction of the axial length of the stent which may be up to 15% of the initial device length. Excessive axial contraction can cause a number of problems in device deployment and performance including difficulty in proper placement and tissue damage. Designs based on ductile hinges 32 can minimize the axial contraction, or foreshortening, of a tissue supporting device during expansion as follows.

FIGS. 9a and 9b illustrate an exaggerated ductile hinge 32 and shortened struts 28 in initial and expanded conditions. Each strut 28 is attached to two ductile hinges 32 at opposite ends. Each ductile hinge 32 has an instant center of rotation  $C_1$ ,  $C_2$  that is an effective pivot point for the attached strut 28. Initially, during expansion the pivot point  $C_1$  is displaced vertically by a distance  $d$  until  $C_1$  is positioned even with  $C_2$  as shown in FIG. 9b. When the array is expanded vertically, the axial struts 28 move in a circular arc with respect to the pivot points, as shown in FIG. 9b. It can be seen that the horizontal distance  $e$  between pivot points  $C_1$  and  $C_2$  actually increases initially, reaching a maximum  $e_{max}$  when the two points are on the same horizontal axis as shown in FIG. 9b. As the vertical expansion continues, the device compresses axially back to its original length. Only when vertical expansion of the array continues beyond the point where the horizontal distance  $e$  between  $C_1$  and  $C_2$  is the same as the original horizontal distance  $e$  does the overall length of the array actually begin to contract.

-24-

For the stent shown in FIG. 2, for example, approximately  $\frac{1}{3}$  of the total circumferential expansion has been accomplished by the time the configuration of FIG. 9b is reached, and the stent exhibits very low axial contraction.

This ability to control axial contraction based on hinge and strut design provides great design flexibility when using ductile hinges. For example, a stent could be designed with zero axial contraction.

An alternative embodiment that illustrates the trade off between crush strength and axial contraction is shown in FIG. 10. FIG. 10 shows a portion of a tissue supporting device 70 having an array of struts 72 and ductile hinges 74 in the unexpanded state. The struts 72 are positioned initially at an angle  $\theta_1$  with respect to a longitudinal axis X of the device. As the device is expanded radially from the unexpanded state illustrated in FIG. 10, the angle  $\theta_1$  increases. In this case the device contracts axially from the onset of vertical expansion throughout the expansion. Once the device has been completely expanded the final angle  $\theta_1$  made by the strut 72 with the horizontal will be much greater than the angle  $\theta$  in the device of FIG. 8a and 8b. As shown previously, a higher final strut angle  $\theta_1$  can significantly increase crush strength and decrease circumferential recoil of the stent structure. However, there is a trade off between increased crush strength and increase in axial contraction.

According to one example of the present invention, the struts 72 are positioned initially at an angle of about  $0^\circ$  to  $45^\circ$  with respect to a longitudinal axis of the device. As the device is expanded radially from the unexpanded state illustrated in FIG. 10a, the strut angle increases to about  $20^\circ$  to  $80^\circ$ .

According to one alternative embodiment of the present invention, the expandable tissue supporting device can also be used as a delivery device for certain beneficial agents including drugs, chemotherapy, or other agents. Due to the structure of the tissue supporting device incorporating ductile hinges, the widths of the struts can be substantially larger than the struts of the prior art devices. The struts due to their large size can be used for beneficial agent delivery

-25-

by providing beneficial agent on the struts or within the struts. Examples of beneficial agent delivery mechanisms include coatings on the struts, such as polymer coatings containing beneficial agents, laser drilled holes in the struts containing beneficial agent, and the like.

While the invention has been described in detail with reference to the preferred embodiments thereof, it will be apparent to one skilled in the art that various changes and modifications can be made and equivalents employed, without departing from the present invention.

-26-

Claims:

1. An expandable medical device comprising:  
a plurality of elongated beams, the plurality of elongated beams joined together to form a substantially cylindrical device which is expandable from a cylinder having a first diameter to a cylinder having a second diameter, the plurality of elongated beams each having a beam width in a circumferential direction; and  
a plurality of ductile hinges connecting the plurality of beams together in the substantially cylindrical device, the ductile hinges having a substantially constant width in a circumferential dimension along a portion of a hinge length which is at least 1/3 a total hinge length, wherein the hinge width is smaller than the beam width such that as the device is expanded from the first diameter to the second diameter the ductile hinges experience plastic deformation while the beams are not plastically deformed.
2. The expandable medical device according to Claim 1, further comprising an abrupt transition between each of the elongated beams and each of the ductile hinges.
3. The expandable medical device according to Claim 1, further comprising a plurality of axial slots between adjacent elongated beams and a plurality of circumferential slots, wherein the plurality of ductile hinges are each formed between an axial slot and a circumferential slot.
4. The expandable medical device according to Claim 3, wherein the ductile hinges are formed at opposite ends of the circumferential slots.
5. The expandable medical device according to Claim 1, wherein the ductile hinges are each in the shape of a curved prismatic beam.

-27-

6. The expandable medical device according to Claim 5, wherein the curved prismatic beams are positioned such that during stent expansion, tensile strain is distributed along a convex surface of the curved prismatic beam.

7. The expandable medical device according to Claim 1, wherein the plurality of elongated beams are formed of wire and the plurality of ductile hinges are reduced diameter portions of the wire.

8. The expandable medical device according to Claim 1, wherein expansion of the substantially cylindrical device from the first diameter to the second diameter which is at least two times the first diameter results in substantially no axial contraction.

9. The expandable medical device according the Claim 1, further comprising a geometric deflection limiting feature for limiting an amount of bending of the ductile hinges.

10. The expandable medical device according to Claim 9, wherein the geometric deflection limiting feature is a V-shaped notch having side surfaces which contact each other when a maximum amount of bending is reached.

11. The expandable medical device according to Claim 1, wherein the plurality of elongated beams extend substantially axially and a plurality of circumferential beams are each connected at first and second ends to one of the axial beams by a ductile hinge.

12. An expandable medical device comprising:  
a cylindrical tube;  
a plurality of axial slots formed in the cylindrical tube in a staggered

-28-

arrangement to define a network of elongated struts, wherein each of the elongated struts are axially displaced from adjacent struts; and

a plurality of ductile hinges formed between the elongated struts, the ductile hinges allowing the cylindrical tube to be expanded or compressed from a first diameter to a second diameter by deformation of the ductile hinges, the ductile hinges being asymmetrically configured to reach a predetermined strain level upon a first percentage expansion and to reach the predetermined strain level upon a second percentage of compression, wherein the first percentage is larger than the second percentage.

13. The expandable medical device according to Claim 12, wherein the elongated struts have a substantially constant width in a circumferential direction, and the ductile hinges have a width in the circumferential direction which is less than  $\frac{2}{3}$  the width of the struts.

14. The expandable medical device according to Claim 13, wherein a transition between the cross sectional area of the struts and the cross sectional area of the ductile hinges is an abrupt transition which extends less than 10 percent of a length of a strut.

15. The expandable medical device according to Claim 12, wherein the plurality of ductile hinges are curved prismatic beams having a convex side surface and a concave side surface.

16. The expandable medical device according to Claim 12, wherein a ratio of a length of the ductile hinges to a length of the axial struts is 1:6 or less.

-29-

17. The expandable medical device according to Claim 12, further comprising a geometric deflection limiting feature for limiting an amount of bending of the ductile hinges.

18. The expandable medical device according to Claim 12, wherein the ductile hinges are designed to deform plastically upon radial expansion or compression of the expandable medical device while the elongated struts experience no plastic deformation upon radial expansion or compression.

19. The expandable medical device according to Claim 12, wherein the expandable medical device is formed of Nitinol, and the ductile hinges are designed to deform upon radial expansion or compression of the expandable medical device and can be returned to an original configuration by heating.

20. The expandable medical device according to Claim 12, wherein the elongated struts include a beneficial agent for delivery to a patient.

21. An expandable medical device comprising:  
a plurality of elongated beams having a substantially constant beam cross sectional area along a beam length;  
a plurality of ductile hinges connecting the plurality of beams together in a substantially cylindrical device which is expandable or compressible from a first diameter to a second diameter by plastic deformation of the ductile hinges; and  
a plurality of deflection limiting members positioned at a plurality of the ductile hinges to limit the deflection at the ductile hinges.

-30-

22. The expandable medical device according to Claim 21, wherein the deflection limiting members include angled side walls on opposite sides of a ductile hinge which engage one another to limit deflection at ductile hinge.

23. The expandable medical device according to Claim 22, wherein the deflection limiting members are V-shaped notches.

24. An expandable medical device which is visible in x-ray and fluoroscope images, the device comprising:  
a plurality of struts arranged to form an expandable cylindrical tube;  
and  
a plurality of ductile hinges connecting the plurality of struts,  
wherein the struts and ductile hinges have a thickness in a radial direction of the cylindrical tube of at least 0.003 inches (0.0762 mm).


25. The expandable medical device according to Claim 24, wherein the device is formed of stainless steel.

26. The expandable medical device according to Claim 24, wherein the thickness of the struts and ductile hinges is at least 0.005 inches (0.127 mm).





1/9

**FIG. 1**  
PRIOR ART

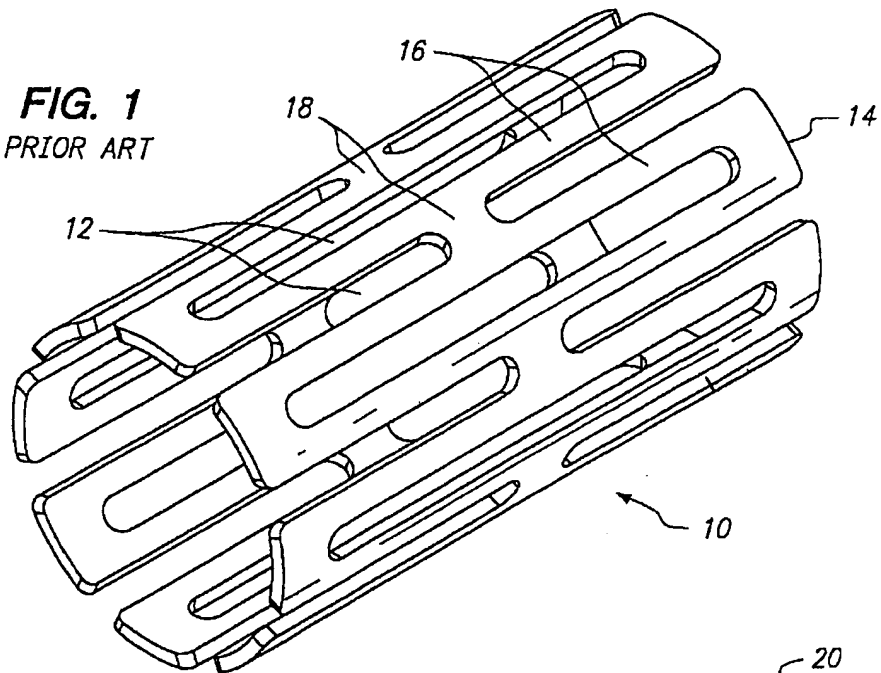


**FIG. 2**

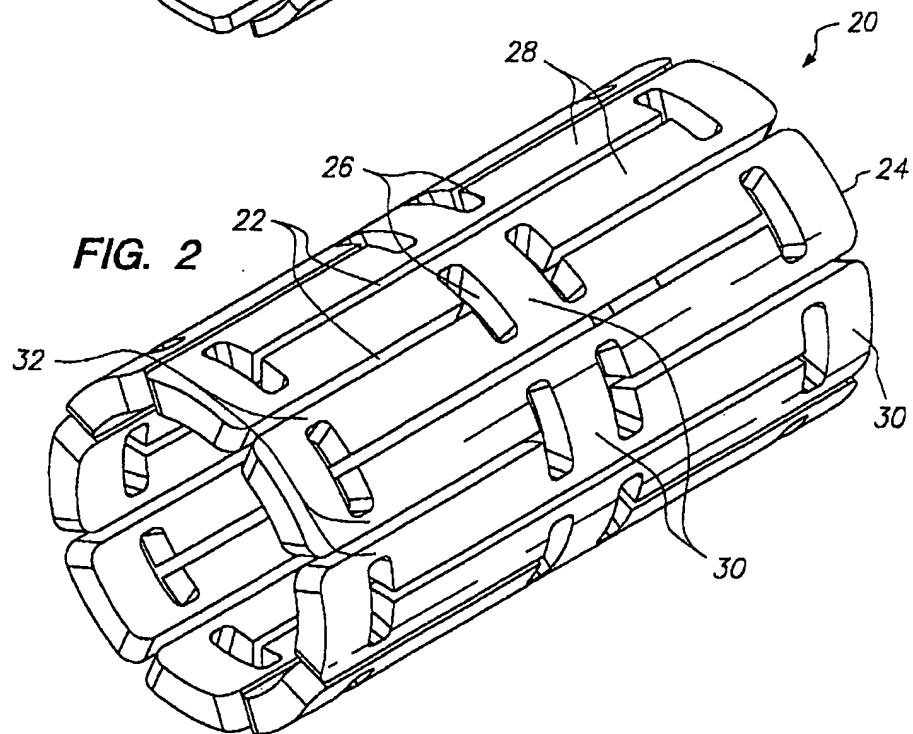


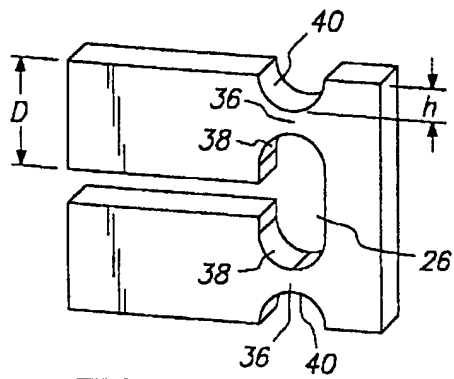


**FIG. 3a**

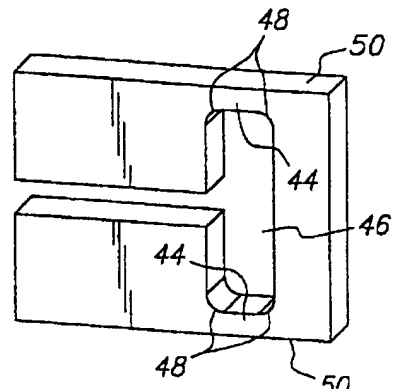

**FIG. 3b**

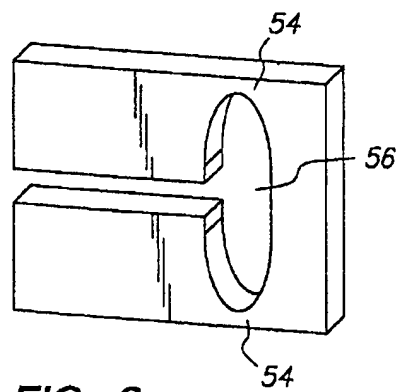

**FIG. 3c**

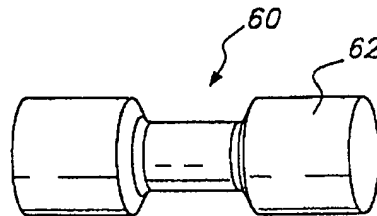

**FIG. 3d**

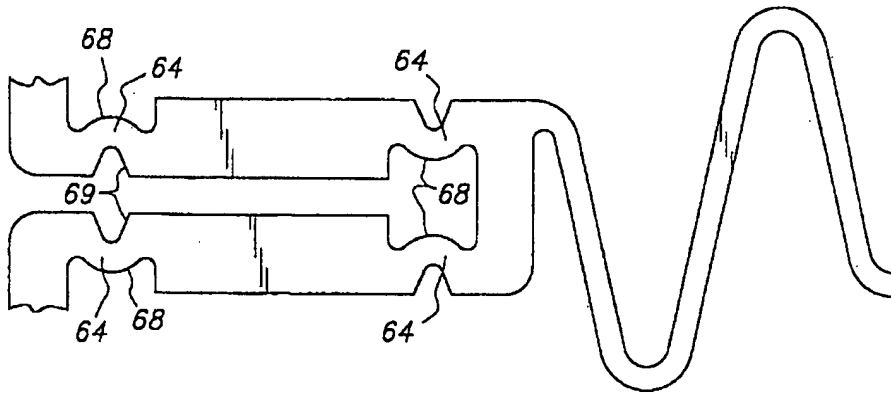


FIG. 3e

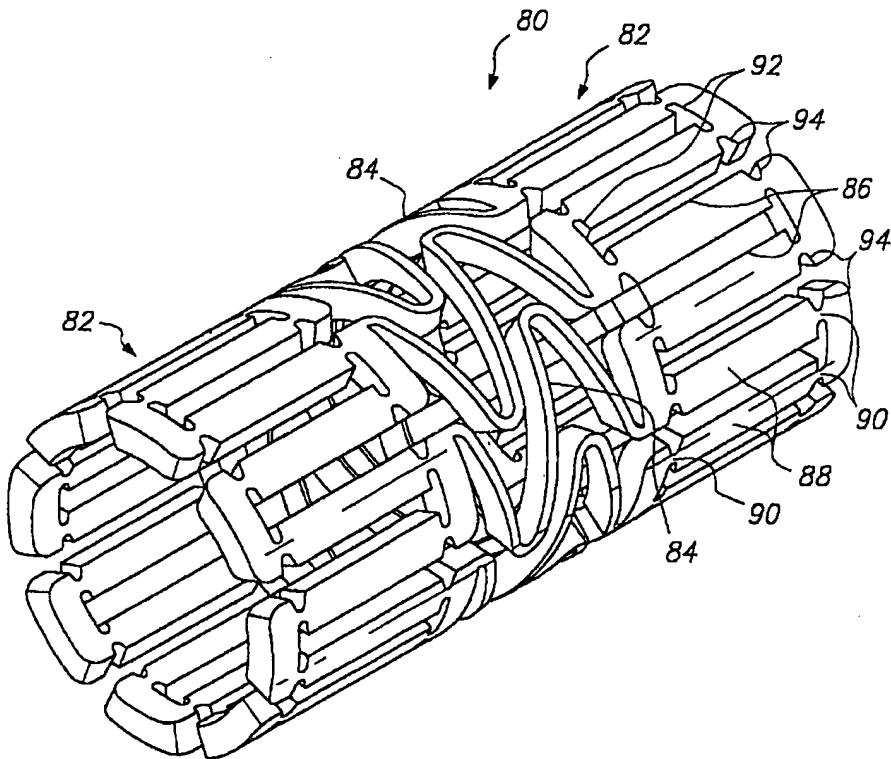


FIG. 4a



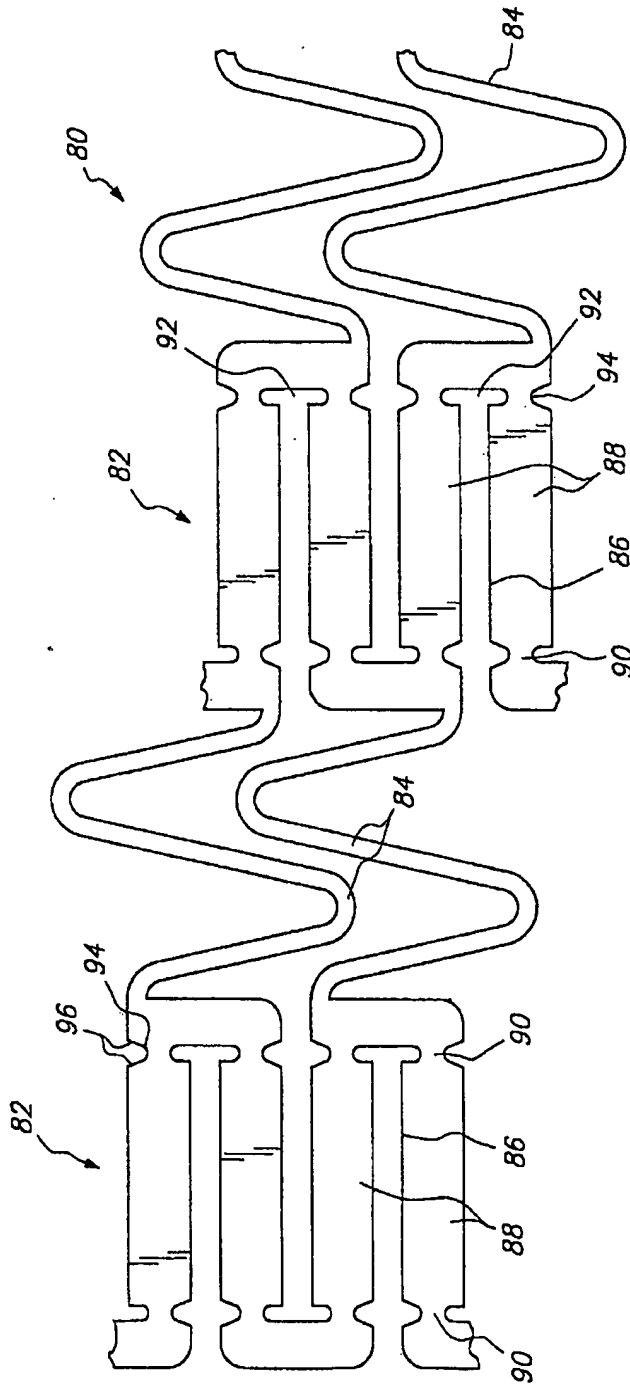



FIG. 4b

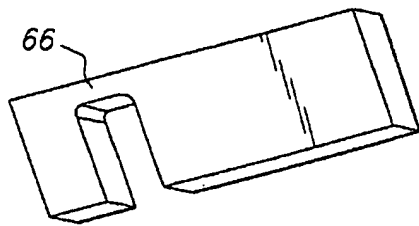


**FIG. 5a**

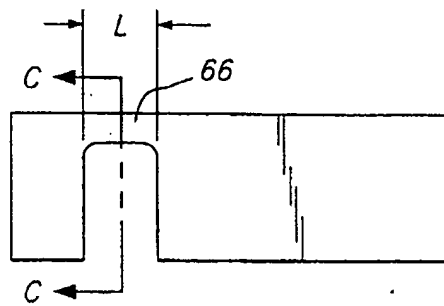

**FIG. 5b**

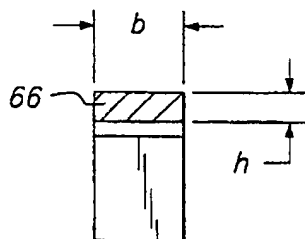

**FIG. 5c**

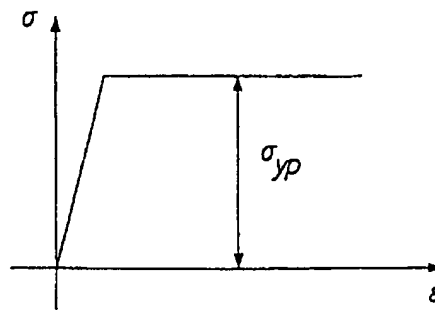

**FIG. 5d**

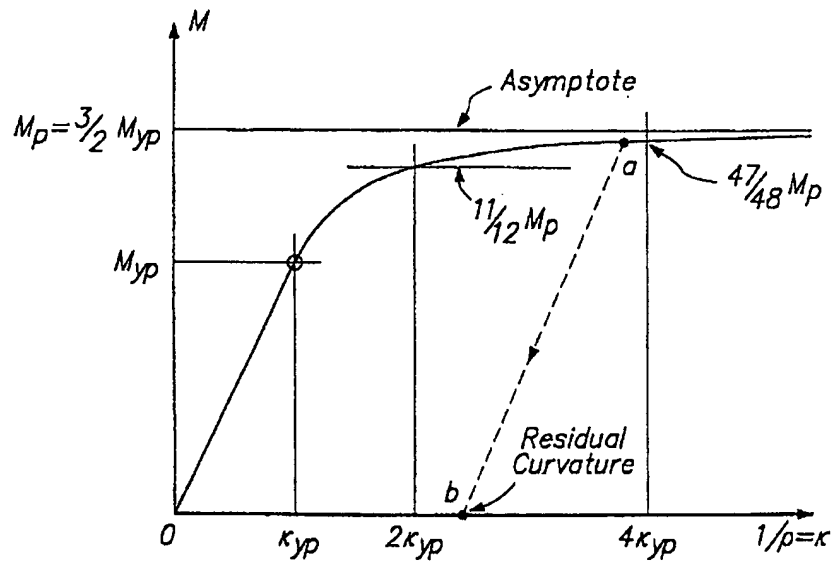
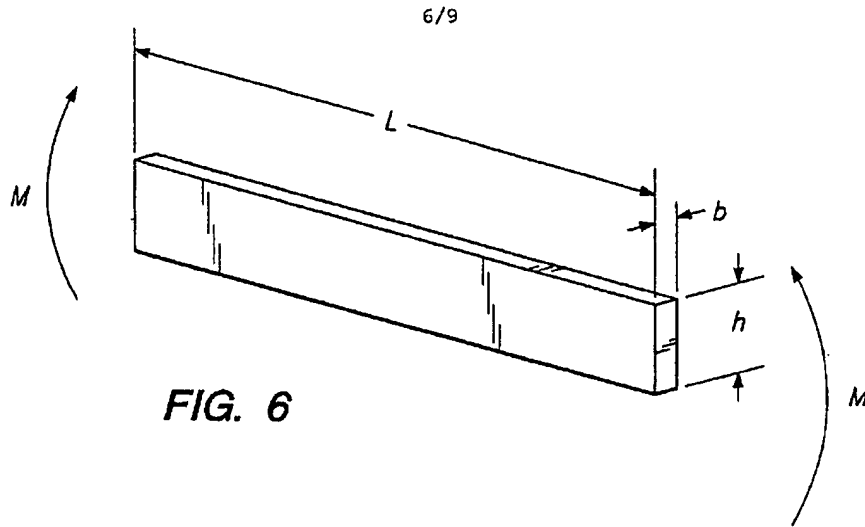


FIG. 7

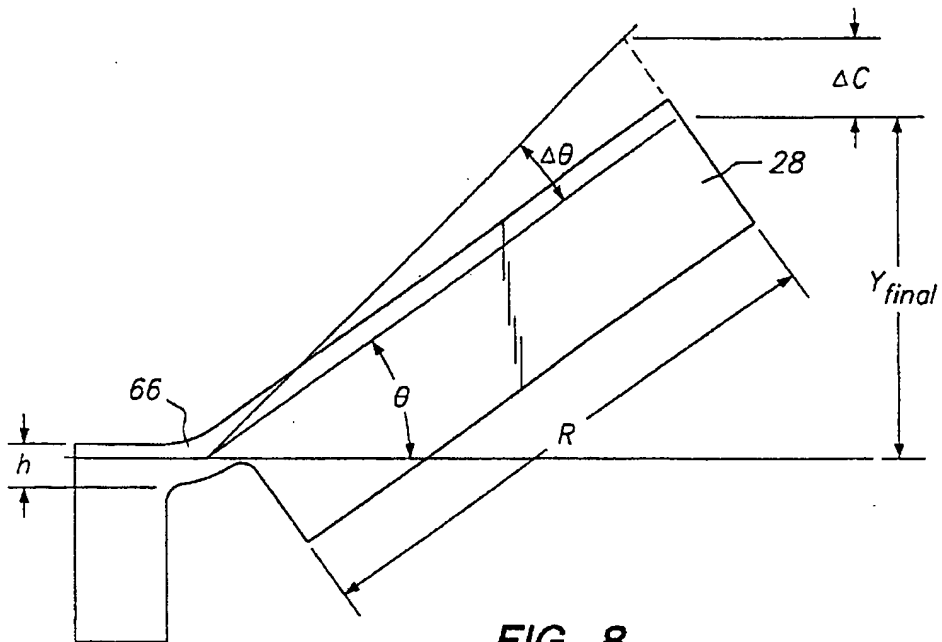


FIG. 8



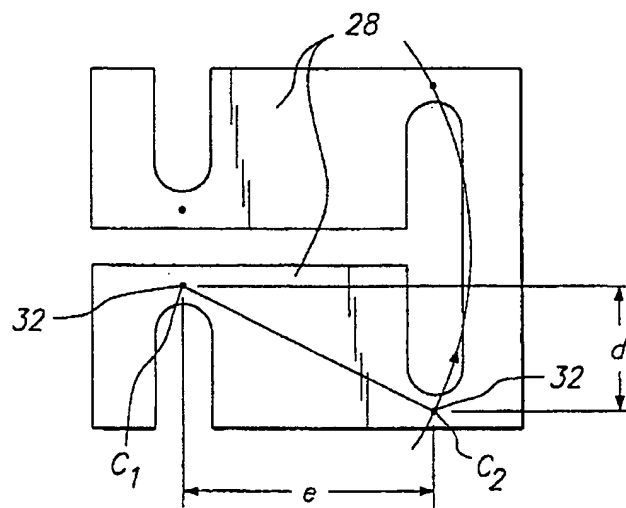


FIG. 9a

**FIG. 9b**

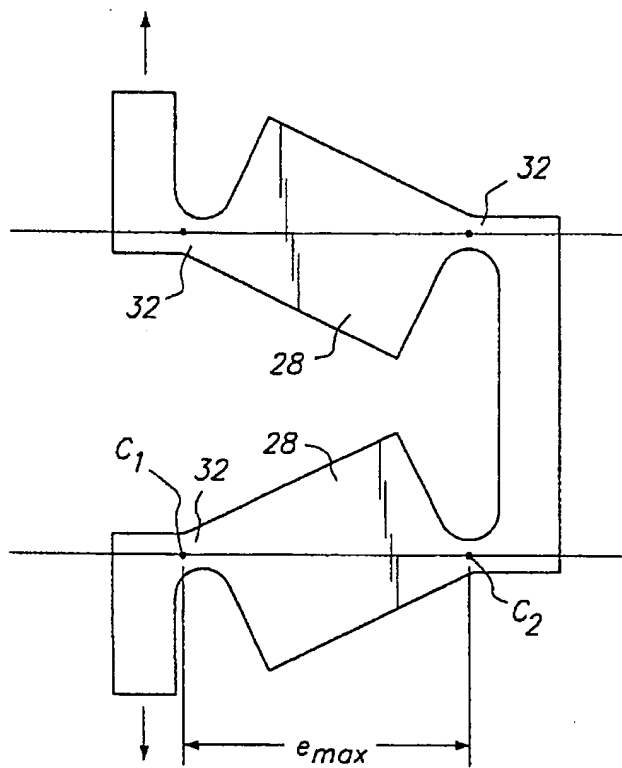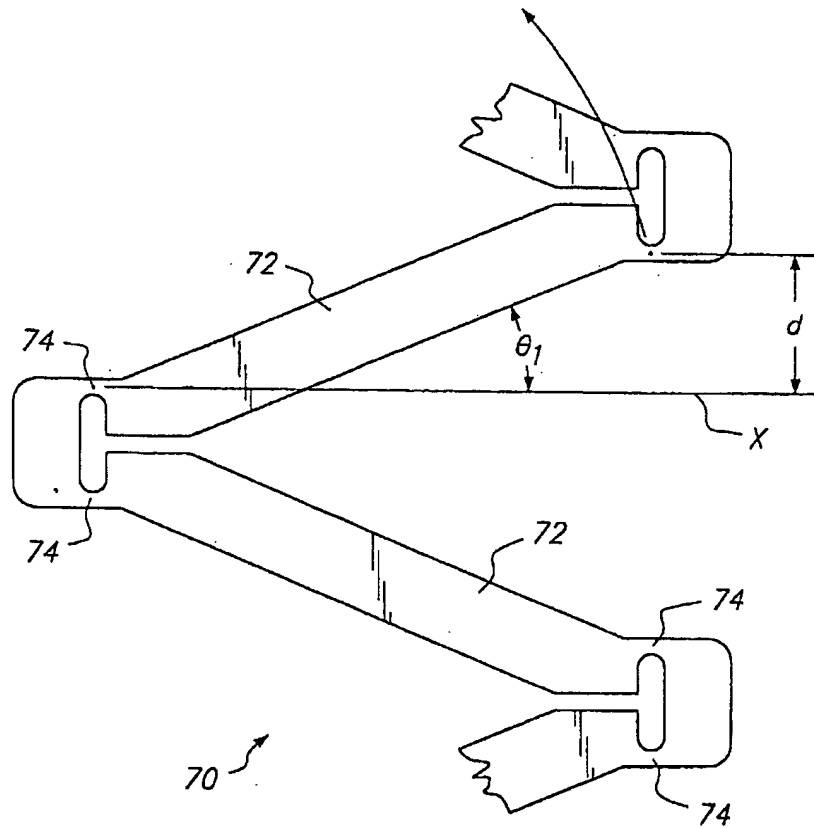

**FIG. 10**

# INTERNATIONAL SEARCH REPORT

International Application No.  
PCT/US 99/06659

A. CLASSIFICATION OF SUBJECT MATTER		
A 61 M 29/00		
According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED		
Minimum documentation searched (classification system followed by classification symbols)		
A 61 F, A 61 M		
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched		
Electronic data base consulted during the international search (name of data base and, where practical, search terms used)		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 96/03092 A1 (BRUN) 08 February 1996, claims 1-12, fig. 1-3. --	1-3, 12
A	US 5383892 A (CARDON et al.) 24 January 1995, claims 1-6, fig. 1. --	1, 12
A	EP 0335341 A (EXPANABLE CRAFTS) 04 October 1989, claims 1, 17, 25, fig. 1A, 7. ----	1-3, 12
<input type="checkbox"/> Further documents are listed in the continuation of box C. <input type="checkbox"/> Patent family members are listed in annex.		
* Special categories of cited documents : "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier document but published on or after the international filing date "L" document which may throw doubt on priority claim(s) or which is cited to establish the publication date of another claim or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art. "&" document member of the same patent family		
Date of the actual completion of the international search		Date of mailing of the international search report
02 June 1999		11. 08. 1999
Name and mailing address of the ISA European Patent Office, P.O. 5818 Patentlaan 1 NL - 2280 HV Rijswijk Tel. (+ 31-70) 340-2040, Tx. 31 631 epo nl, Fax (+ 31-70) 340-3016		Authorized officer MIHATSEK e.h.

## ANHANG

zum internationalen Recherchen-  
bericht über die internationale  
Patentanmeldung Nr.

## ANNEX

to the International Search  
Report to the International Patent  
Application No.

## ANNEXE

au rapport de recherche inter-  
national relatif à la demande de brevet  
international n°

PCT/US 99/04659 SAE 230056

In diesem Anhang sind die Mitglieder  
der Patentfamilien der im obenge-  
nannten internationalen Recherchenbericht  
geführten Patentdokumente angegeben.  
Diese Angaben dienen nur zur Unter-  
stützung und erfolgen ohne Gewähr.

This Annex lists the patent family  
members relating to the patent documents  
cited in the above-mentioned inter-  
national search report. The Office is  
in no way liable for these particulars  
which are given merely for the purpose  
of information.

La présente annexe indique les  
membres de la famille de brevets  
relatifs aux documents de brevets cités  
dans le rapport de recherche inter-  
national visé ci-dessus. Les renseigne-  
ments fournis sont donnés à titre indica-  
tif et n'engagent pas la responsabilité  
de l'Office.

In Recherchenbericht geführtes Patentdokument Patent document cited in search report Document de brevet cité dans le rapport de recherche	Datum der Veröffentlichung Publication date Date de publication	Mitglied(er) der Patentfamilie Patent family member(s) Membre(s) de la famille de brevets	Datum der Veröffentlichung Publication date Date de publication
JD A1 9603092 08-02-1996		AT E 170733	15-09-1998
		AU A1 32706785	22-02-1996
		AU B2 702468	25-02-1999
		BR A 9508383	04-11-1997
		CA AA 2195783	08-02-1996
		CN A 158078	27-08-1997
		CN A3 9700191	11-06-1997
		DE U1 32521205	24-11-1996
		DE U1 32521206	24-11-1996
		DE U1 32521193	05-12-1996
		DE T 195581503	16-01-1997
		DE T2 195581503	02-04-1998
		DE T2 69304659	15-10-1998
		DE T2 69304659	06-09-1999
		DK A 180797	19-02-1997
		EP A1 762856	19-03-1997
		EP A4 762856	04-04-1997
		EP A2 8464448	10-06-1998
		EP A2 8464449	10-06-1998
		EP A2 8464450	10-06-1998
		EP A2 8464451	10-06-1998
		EP A2 8464452	10-06-1998
		EP B1 762856	09-09-1998
		EP J 4424800	21-01-1997
		EP A 703166	07-01-1997
		EP A 9703166	07-03-1997
		EP A 9701689	19-03-1997
		EP A 9701689	26-03-1997
		EP A 9721568	10-13-1997
		EP A 9721568	04-02-1998
		EP A 9704587	15-07-1998
		EP A 9704587	19-07-1998
		EP A 10503676	07-04-1998
		EP A 970031	16-04-1997
		EP A 970289	23-01-1997
		EP A 970289	26-03-1997
		EP A 18270	26-05-1997
		EP A 9700206	24-01-1997
		EP A 9700206	28-02-1997
		EP A 9520079	31-12-1997
		EP A 115797	08-10-1997
		US A 5733303	01-03-1998
		US A 5843120	01-12-1998
		US A 97032	29-11-1997
		US B 4377	25-08-1998
		US AA 2249488	21-10-1996
		US A 5449373	12-09-1998
		US A 9633671	31-10-1996
		US A 24279795	18-11-1996
		US A 9703400	17-06-1998
		US T 195581506	21-08-1997
		US A 9703400	29-10-1997
		US A 974062	19-10-1997
		US A 12036	20-05-1998
		US A 974938	16-10-1997
		US A 974938	16-12-1997
		US A 11501551	02-03-1998
		US T2 11501551	09-02-1999
		US A 1457797	07-10-1998
		US A 9510585	05-01-1999
		NZ A 285241	29-03-1999
S A 5383892 24-01-1993		AT E 133554	15-02-1996
		CA AA 2082367	09-05-1996
		DE T2 69208026	14-03-1996
		DE T2 69208026	05-09-1996
		DK T3 541443	03-06-1996
		EP A1 541443	12-05-1996
		EP B1 541443	31-01-1996
P A1 335341 04-10-1989		FR T3 2085599	01-06-1996
		FR A1 2583449	14-05-1993
		US A 5102417	07-04-1992
		AT A 7064	15-03-1992
		AU A1 31742789	28-09-1989
		AU B2 623498	04-02-1993
		CA A1 1830186	14-06-1994
		DE CO 68900895	09-04-1992

US	A	1330186	14-06-1994
US	A	68900893	09-04-1992
US	A	335841	24-03-1992
US	A	2030230	06-04-1992
US	A	3003986	06-04-1992
US	A	1299980	04-04-1992
US	A	9711750	10-07-1997
US	A	9711751	10-07-1997
US	A	9711752	10-07-1997
US	A	8902387	27-12-1989
US	A	60500	15-02-1991
US	A	64882786	14-06-1997
US	A	591942	24-03-1992
US	A	8605658	18-04-1997
US	A	1281504	18-04-1997
US	A	1381505	18-04-1997
US	A	1381506	07-05-1996
US	A	3677221	07-05-1997
US	A	221570	17-05-1997
US	A	221570	27-12-1989
US	A	221570	27-12-1989
US	A	3001410	20-01-1991
US	A	62231657	20-01-1991
US	A	4006377	15-10-1987
US	A	4357949	05-02-1992
US	A	9276302	10-12-1992
US	A	2731642	28-10-1997
US	A	4733665	28-03-1998
US	A	4733665	29-03-1998
US	A	8608414	11-01-1994
US	A	4739762	30-09-1987
US	A	4776337	26-04-1988
US	A	4739762	11-10-1988
US	A	4739762	27-10-1998

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☒ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**